

FIG.1

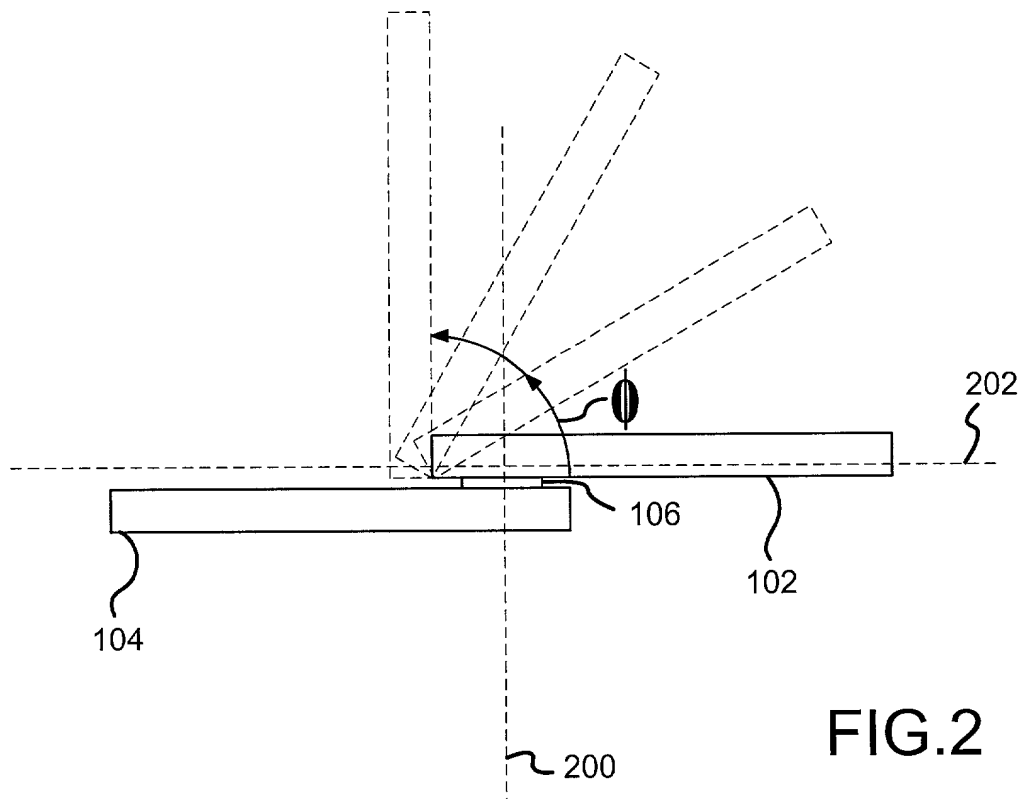


FIG.2

FIG. 3 is a perspective view of the device 100 in a closed position.

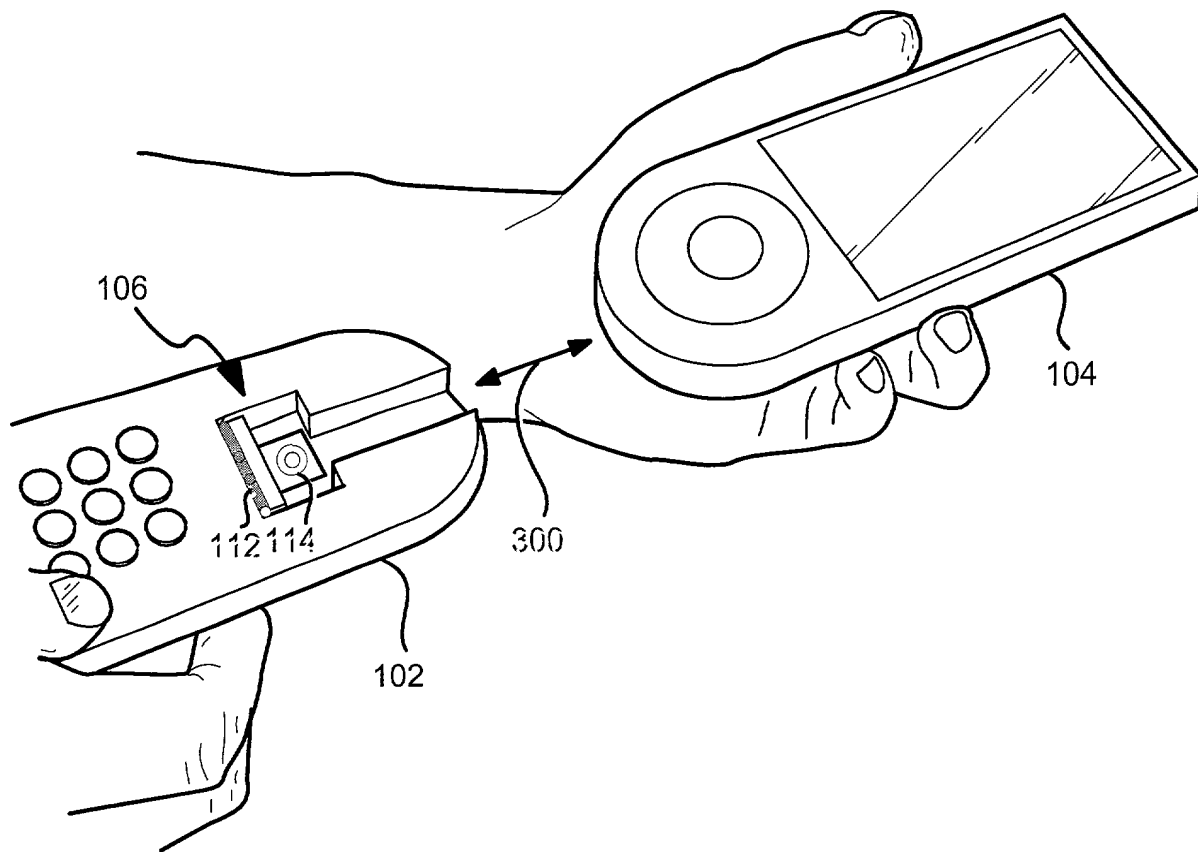


FIG.3

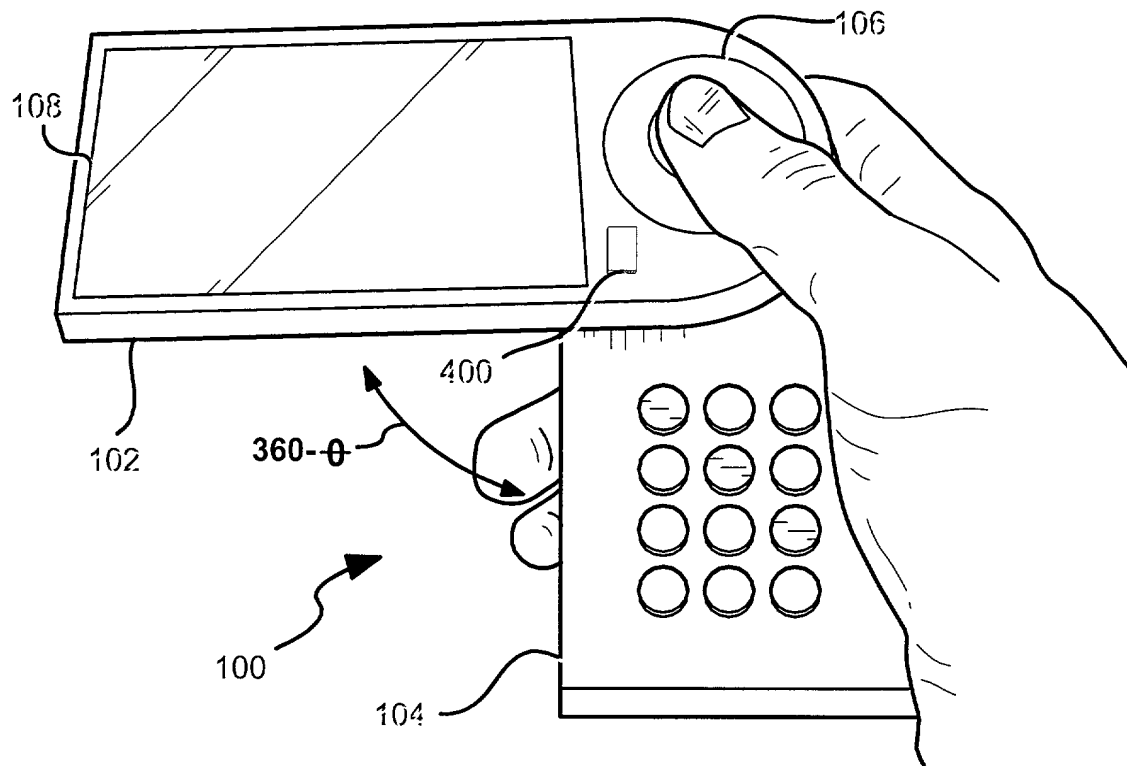


FIG. 4A

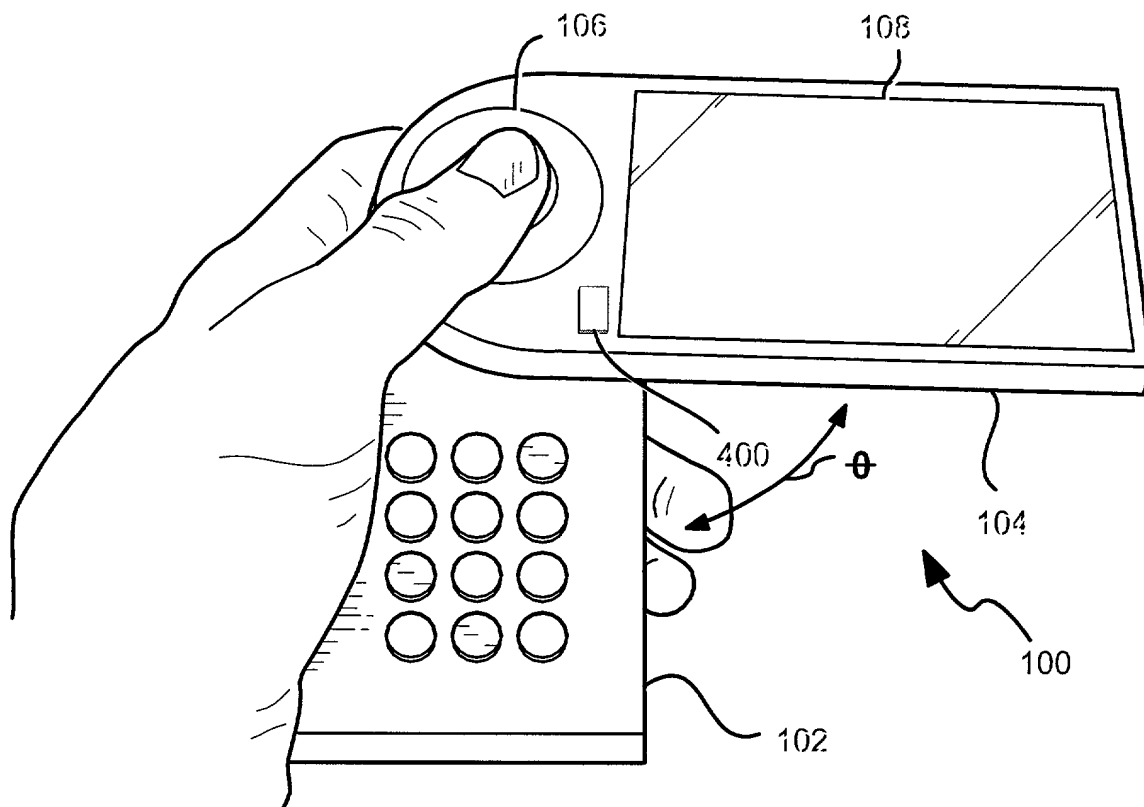
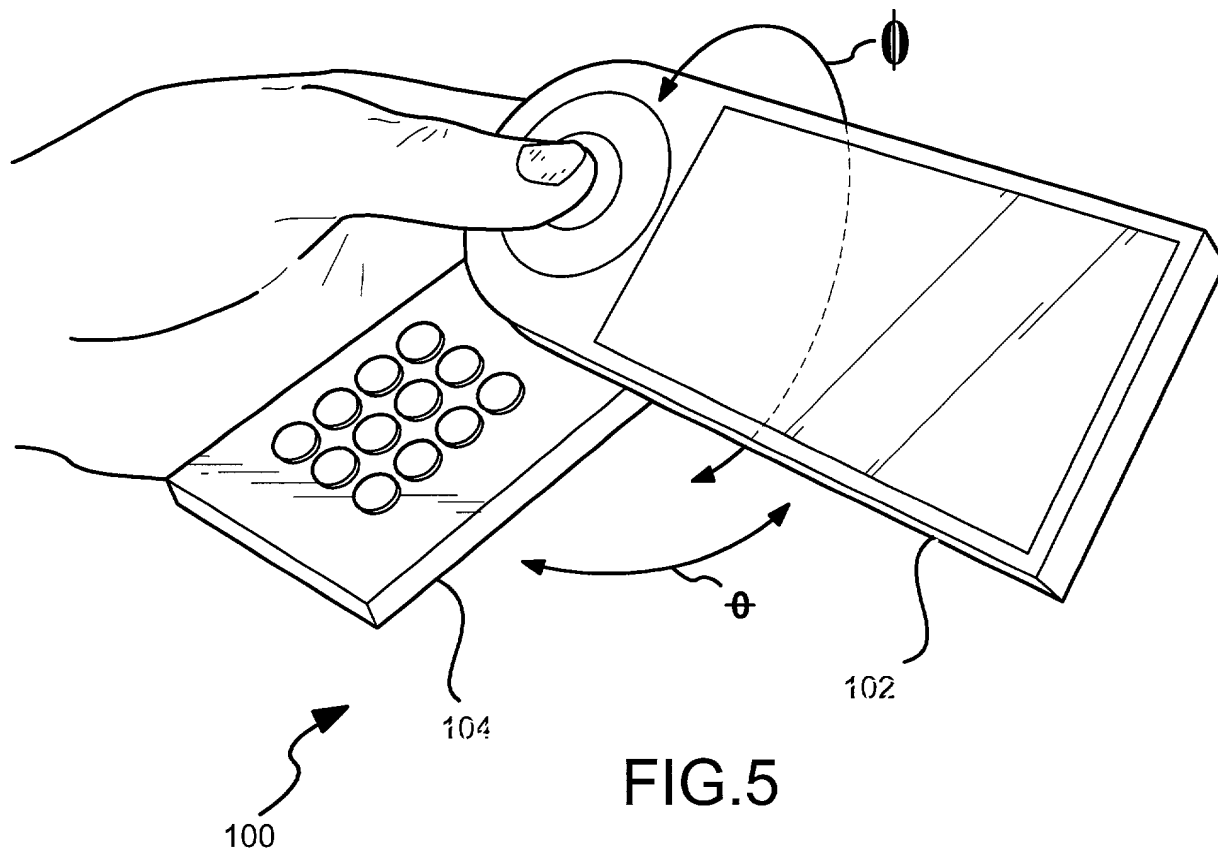


FIG. 4B



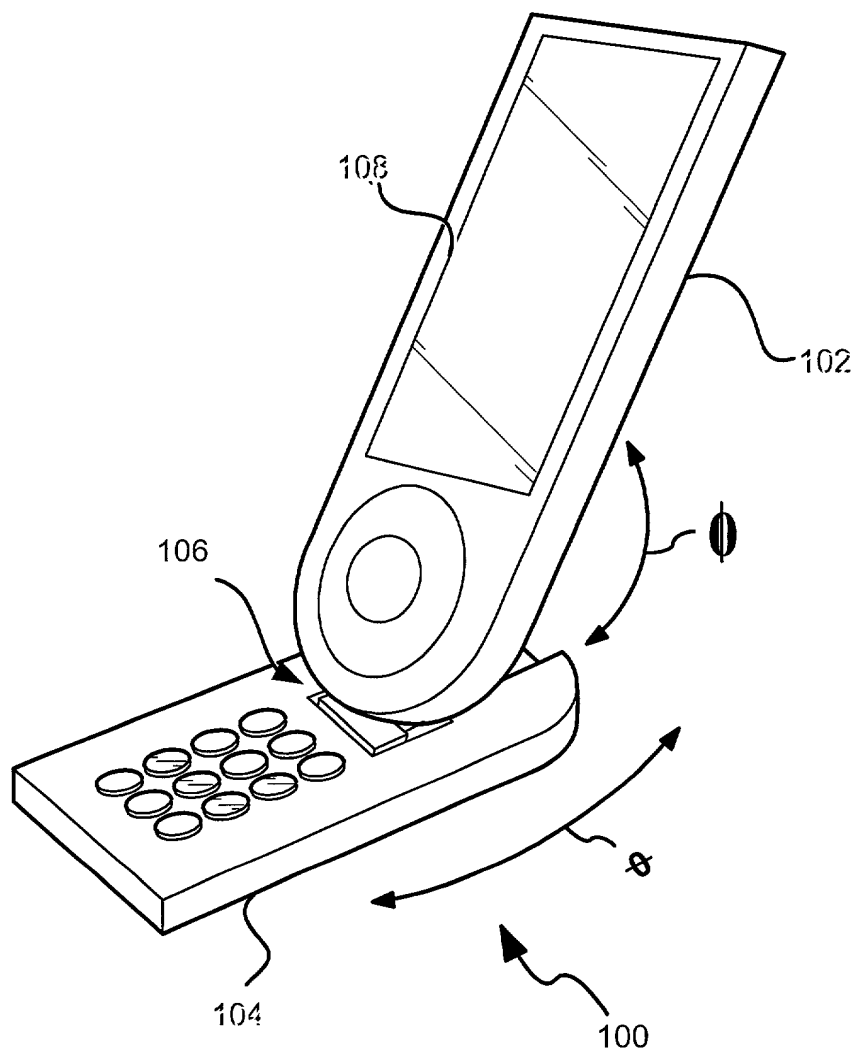


FIG.6